

Product Class	Test Item	Specimen Type	Specimen Volume	Reaction Time	Measuring Range	Clinical Reference	Qualification
Vitamin	Vitamin D	Serum/Plasma	75 µL	15 min	5-100 ng/mL	30-100 ng/mL	CE
Diabetic & Renal Injury Markers	HbA1c	WB	10 µL	5 min	4.0-14.5%	4-6.5%	CE IFCC NGSP
	MAU	Urine	75 µL	3 min	5-300 mg/L	0-20 mg/L	CE
	NGAL	Urine	75 µL	15 min	10-1500 ng/mL	≤131.7 ng/mL	CE
Thyroid Function	T3	WB/Serum/Plasma	75 µL	15 min	0.61-9.22 nmol/L	1.23-3.07 nmol/L	CE
	T4	WB/Serum/Plasma	75 µL	15 min	12.87-300 nmol/L	66-181 nmol/L	CE
	TSH	WB/Serum/Plasma	75 µL	15 min	0.1-100 mIU/L	0.3-4.2 mIU/L	CE
	fT3 ^{New}	WB/Serum/Plasma	75 µL	15 min	0.40-50.00 pmol/L or 0.26-32.55 pg/mL	2.8-7.1 pmol/L (1.82-4.61 pg/mL)	CE
	fT4 ^{New}	WB/Serum/Plasma	75 µL	15 min	1.00-100 pmol/L or 0.078-7.77 ng/dL	12-22 pmol/L (0.94-1.72 ng/dL)	CE
Fertility	β-HCG	WB/Serum/Plasma	20 µL	15 min	2-200,000 mIU/mL	5 mIU/mL	CE
	LH	WB/Serum/Plasma	75 µL	15 min	1-100 mIU/mL	Male: 1.70-8.60 mIU/mL; Female: Follicular phase: 2.95-13.65 mIU/mL Ovulation phase: 13.65-95.75 mIU/mL Luteal phase: 1.25-11.00 mIU/mL Menopause phase: 8.24-55.23 mIU/mL	CE
	FSH	WB/Serum/Plasma	75 µL	15 min	1-100 mIU/mL	Male: 1.50-12.40 mIU/mL Female: Follicular phase: 4.46-12.43 mIU/mL Ovulation phase: 4.85-20.96 mIU/mL Luteal phase: 1.96-7.70 mIU/mL Menopause phase: 22.70-130.00 mIU/mL	CE
	Prog	WB/Serum/Plasma	75 µL	15 min	1.5-60 ng/mL	Male: 0.2-1.5 ng/mL Female: Follicular phase: 0.2-2.0 ng/mL Ovulation phase: 0.7-3.5 ng/mL Luteal phase: 3.0-30 ng/mL Menopause phase: 0.1-0.9 ng/mL 7 weeks of pregnancy: 24.5±7.6 ng/mL 9-12 weeks of pregnancy: 38.0±13.0 ng/mL	CE
	PRL	WB/Serum/Plasma	75 µL	15 min	1-200 ng/mL	Female (non-pregnant): 4.60-25.07 ng/mL Male: 3.45-17.42 ng/mL	CE
	E2	WB/Serum/Plasma	75 µL	15 min	9-3000 pg/mL	Male: <85 pg/mL Female: Follicular Phase: 12-262 pg/mL Ovulation: 40-396 pg/mL Luteal Phase: 21-361 pg/mL Menopause: <190 pg/mL Pregnancy: >145 pg/mL	CE
	Testosterone	WB/Serum/Plasma	75 µL	15 min	0.2-15 ng/mL	Male: 20-49 years old: 1.61-8.41 ng/mL ≥50 years old: <0.61 ng/mL Female: 20-49 years old: 0.80 ng/mL ≥50 years old: <0.71 ng/mL	CE
Cardiac Markers	NT-proBNP	WB/Serum/Plasma	75 µL	15 min	18-35000 pg/mL	<75 years old: 0-300 pg/mL ≥75 years old: 0-450 pg/mL	CE
	cTn I	WB/Serum/Plasma	75 µL	15 min	0.1-50 ng/mL	0-0.3 ng/mL	CE
	Myo	WB/Serum/Plasma	75 µL	15 min	2.0-400 ng/mL	0-58 ng/mL	CE
	CK-MB	WB/Serum/Plasma	75 µL	15 min	0.3-100 ng/mL	0-5 ng/mL	CE
	3 in 1 (cTn I/Myo/CK-MB)	WB/Serum/Plasma	75 µL	15 min	Same with single items	Same with single items	CE
	BNP	WB/Plasma	75 µL	15 min	5-5000 pg/mL	0-100 pg/mL	CE
Coagulation	D-Dimer	WB/Plasma	15 µL for whole blood 10 µL for plasma	5 min	0.1-10 mg/L	0-0.5 mg/L	CE
	D-Dimer one step	WB/Plasma	100 µL for whole blood 75 µL for plasma	15 min	0.1-10 mg/L	0-0.5 mg/L	CE
Inflammation Markers	PCT	WB/Serum/Plasma	75 µL for whole blood 50 µL for plasma/serum	15 min	0.1-100 ng/mL	0-0.5 ng/mL	CE
	CRP (hsCRP+CRP)	WB/Serum/Plasma	8.5 µL for whole blood 5 µL for plasma/serum	3 min	0.5-200 mg/L	CRP: 0-10 mg/L hsCRP: 0-1 mg/L	CE
	SAA	WB/Serum/Plasma	10 µL	15 min	1.0-300 mg/L	0-10 mg/L	CE
Tumor Markers	AFP	WB/Serum/Plasma	75 µL	15 min	5-400 ng/mL	0-20 ng/mL	CE
	PSA	WB/Serum/Plasma	75 µL	15 min	2-100 ng/mL	0-4 ng/mL	CE 9123
	CEA	WB/Serum/Plasma	75 µL	15 min	1-500 ng/mL	0-5 ng/mL	CE
	fPSA	WB/Serum/Plasma	75 µL	15 min	0.2-30 ng/mL	< 1 ng/mL	CE 9123
Others	Cortisol	WB/Serum/Plasma	75 µL	15 min	50-1000 nmol/L	7:00-10:00 a.m.: 201.31-536.54 nmol/L 4:00-8:00 p.m.: 65.78-330.85 nmol/L	CE

Wondfo®

Finecare™ FIA Meter (FS-112)

Fluorescence Immunoassay Rapid Quantitative Test

- Rapid
- Accurate
- Convenient
- Reliable
- Popular
- Extensible



Wondfo

Guangzhou Wondfo Biotech Co., Ltd.
 Add: No. 8 Lizhishan Road, Science City, Luogang District, 510663, Guangzhou, P.R. China
 Tel: +86-20-32296083 Fax: +86-20-32296063
 E-mail: sales@wondfo.com.cn Websites: www.en.wondfo.com.cn

Rev. A5 Rel.: 2020/04/27

GUANGZHOU WONDFO BIOTECH CO., LTD.



Finecare™ FIA Meter

Finecare™ FIA Meter is a fluorescence immunochromatographic analyzing system which can help diagnose conditions such as inflammation, diabetes, cardiovascular diseases, renal injury and cancers, etc.

The Finecare™ platform provides reliable and quantitative results of various kinds of analytes in human blood or urine within several minutes.

Application: Laboratory, ER, Cardiology, ICU, Respiratory, Pediatrics, etc.

Test Item

● Metabolic Markers

Vitamin D

● Thyroid Function

TSH, T3, T4, fT3, fT4

● Inflammation Markers

CRP+hsCRP, PCT, SAA

● Coagulation

D-Dimer, D-Dimer one step

● Tumor Markers

PSA, fPSA, AFP, CEA

● Diabetic & Renal Injury Markers

HbA1c, MAU, NGAL

● Fertility

β-HCG, FSH, LH, Prog, Testosterone, PRL, E2

● Cardiac Markers


cTnI, CK-MB, Myo, NT-proBNP, BNP,

cTnI/CK-MB/Myo

● Others

Cortisol

Principle and Operation

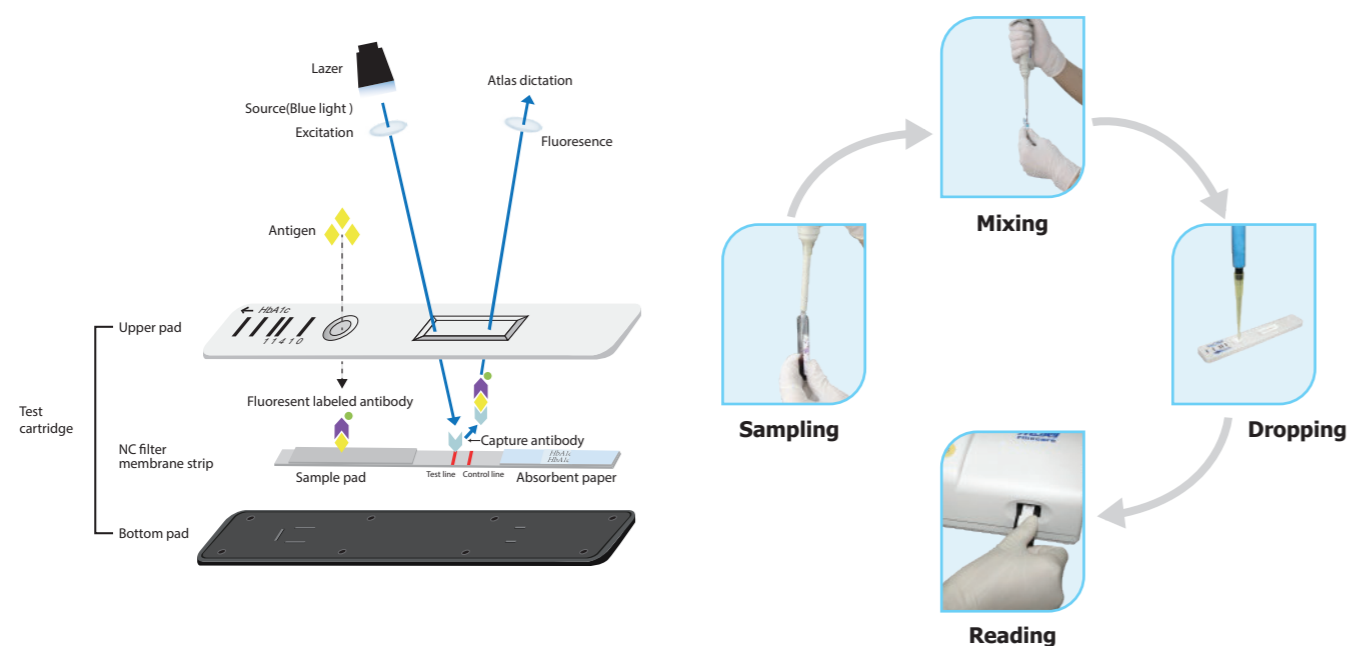

Why Choose Finecare™



Extra quick operating mode for large number of specimens



Powerful information management (Direct connection to LIS/HIS)



Convenient and fast. Get results in 3-15 minutes

Unique quick mode

Designed sampler

Information management


Reliable accuracy

Instant result


Room temperature storage



Specially-designed sampler for small volume of specimen

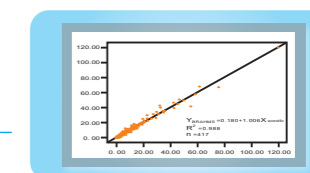

Good correlation with wet chemistry method results

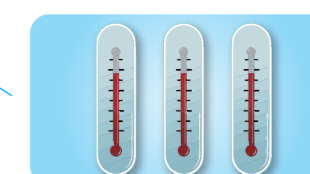

Solid synthetic craft, can be stored at room temperature (4-30℃)

Built-in Thermal Printer

Real-time printing

3.5" LCD Touch Screen

Dimensions:
250(L) x 258(W) x 104(H)mm
Weight:
2.5kg
Power adapter:
100-240AC, 50-60Hz

LIS Connection

Direct connection to LIS / HIS

ID Chip Port

The ID chip contains all information of test item and lot number

Test Channel

The Test Cartridge Holder

